

---

Sample Preparation

---

Automated Sonication


---

POC

---

*The 8100S combines high energy sonication with an XYZ autosampler, ensuring the contents of a sample vial are quickly and thoroughly homogenized prior to analysis*

*Combine the 8100S automated sonication system with a TOC analyser to measure the Particulated Organic Carbon fraction of an aqueous sample (POC)*

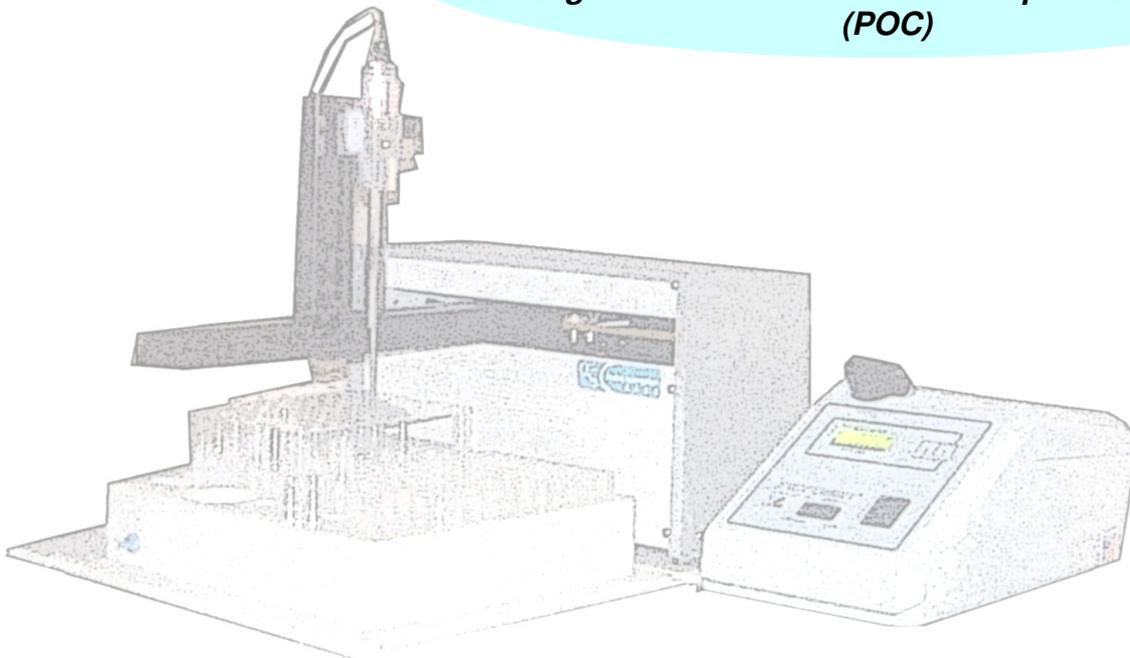

## Automated Sample Homogenization

---

***Fast and Complete***

